

NEITZ

Binocular Indirect Ophthalmoscope *IO-α / IO-α LED*

POWERSOURCE	BATTERY PACK	TRANSFORMER
IO-α	BP-Li <ul style="list-style-type: none"> • Consecutive Use Time : About 80 min. • Full Charging Time : 2hours • Dimension : 48x83x49 (mm) • Weight : 183g 	PSU-3K <ul style="list-style-type: none"> • Voltage Input : AC 120V or 230V. • Dimension : 158x100x90 (mm) • Weight : 1200g 
IO-α LED	IO-BPII <ul style="list-style-type: none"> • Consecutive Use Time : About 5 hours / Max, About 10 hours / Middle • Full Charging Time : 2.5hours • Dimension : 72.5x65x20 (mm) • Weight : 140g 	LPS-250 <ul style="list-style-type: none"> • Voltage Input : AC 120V or 230V. • Dimension : 158x100x90 (mm) • Weight : 500g 

ACCESSORIES

Accessories included are Different depending on the set.



Teaching mirror

Carrying case

Detachment chart and head pad

OPTION



PSU-S
Transformer and PSU-S,
Transformer Stand

Aspherical Viewing Lens 20D

2400RS
Lithium Ion Battery for Battery Pack BP-Li

Lamp House Conversion Kit
• Lamp House with 0.6M cord
• Extension Curl cord



NEITZ

NEITZ INSTRUMENTS CO., LTD.
4F Ichibancho Court, 15-21 Ichibancho,
Chiyoda-ku, Tokyo 102-0082, Japan
Tel: +81-3-3237-0552 Fax: +81-3-3237-0554



NEITZ pursues Comfort and Flexibility. Everything is for Your Best Performance.

Fundus image can be observed stereoscopically even through a small pupil of 2 mm diameter.

Observation angle can be continuously changed. Smooth single hand adjustment of mirrors allows the observation easily in any desired angle.

The halogen light provides suitable illumination for general observation.

Specifications

Pupillary Distance : 54mm to 74mm
 Illumination Area : Φ 19mm, Φ 50mm,
 Φ 80mm (at the distance of 500mm)
 Filters : UV, Blue, Red-Free
 Light Source : L-51 Halogen Bulb
 Dimensions : 230mm (w) x 310mm (D) x 250mm (H)
 Weight : 480g



New LED Light source reproduces clean illumination in Halogen bulb color and eliminates the filament shadow.

LED light source provides steady illumination for 50,000 hours, free from exchange the light bulb.

The combination of the LED and the powerful re-chargeable battery allows 5 times longer operation and 10 hours continuous lighting.


Specifications

Pupillary Distance : 54mm to 74mm
 Illumination Area : Φ 19mm, Φ 50mm,
 Φ 80mm(at the distance of 500mm)
 Filters : UV, Blue, Red-Free
 Light Source : 3W White LED
 Dimensions : 230mm (W) x 310mm (D) x 250mm (H)
 Weight : 480g




OPTICS SYSTEM

The Illumination Light Mirror and Observation Mirrors are adjustable respectively with a single hand.

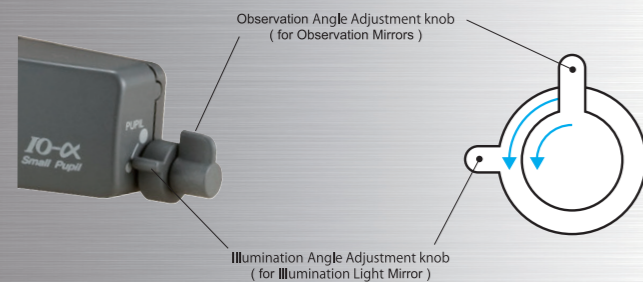


Small pupil

Clear stereoscopic fundus image can be easily obtained through small pupil with the mirrors.

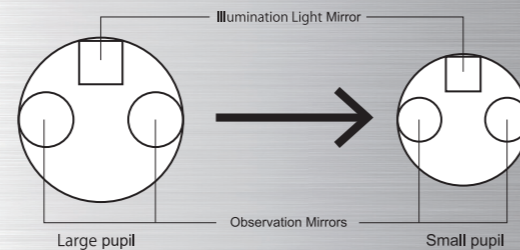


Freedom in choice of the approach angle to the pupil.

The system allows to adjust the position of the mirrors into vertical or horizontal positions corresponding to the patient pupil. It enables the operator to observe the periphery of the patient fundus from any angle.

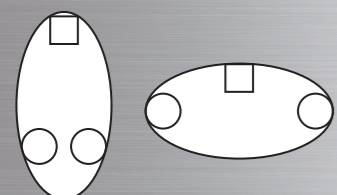


The optical system of Neitz IO-a can position the mirrors into either vertical or horizontal oblong in corresponding to available observation angle for the operator at examination.




The area, the periphery of fundus, is difficult to be observed in some approach angle to the pupil unless the optical system can position the mirrors like Neitz IO-α.

HALOGEN BULB COLOR LED



Characteristic of our LED (in comparison with white color LED)

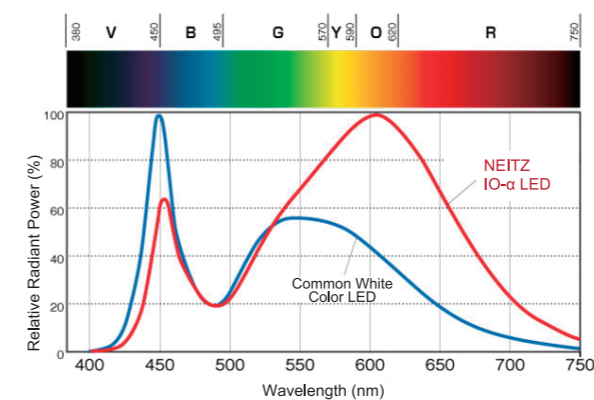

The color temperature of the LED of Neitz IO-a LED is 3200°K, which is same color temperature to the halogen bulb used in the typical binocular indirect ophthalmoscope.

The colors observed in ophthalmology are red of blood vessel, orange of retina and yellow of optic disc. Differently from common white color LED used in the binocular indirect ophthalmoscopes of other manufacturers, our halogen bulb color LED reproduces these colors with high color rendering properties as shown in the chart on the left. It supports operator to obtain the maximized information from the fundus observation for more precise diagnosis.

It enables to observe fundus under the same condition of illumination compatible to the halogen bulb illumination of familiar.